	<b>CALIBRATION CERTIFICATE</b>		Document No:		CALCERT-ASY-0762C-SN-10183528		
			Rev No:	A	Date:	10 JUL 2014	
	<b>CONFIDENTIAL</b>		Page 1 of 1		Authorized By:		S. ANTE
			Released By:		2288		

## FOCUS® PROBE CALIBRATION CERTIFICATE

DOCUMENT NAME:

CALCERT-ASY-0762C-SN-10183528

DATE:

30 JAN 2015

### 1. PRODUCT ID

MANUFACTURER:

Photon Control Inc.

MODEL#:

OFH-INS-3/4-SS-HP-HYB

PART#:

ASY-0762C

SERIAL#:

10183528

CORRECTION TABLE:

CAL-FIT-INS-148B-NPS6-1R-NOFC-002-10

### 2. TEST

PROCEDURE:

CALPROC-ASY-0762C

METHOD:

COMPARISON

MEDIUM:

AIR

TEMPERATURE:

20°C

PRESSURE:

101.85 kPaA


RANGE:

0.1 – 12 m/s

REFERENCE TEST EQUIPMENT:

ABB Total Sonic TS 9048 D-1, SN-04148715

### 3. TEST RESULTS

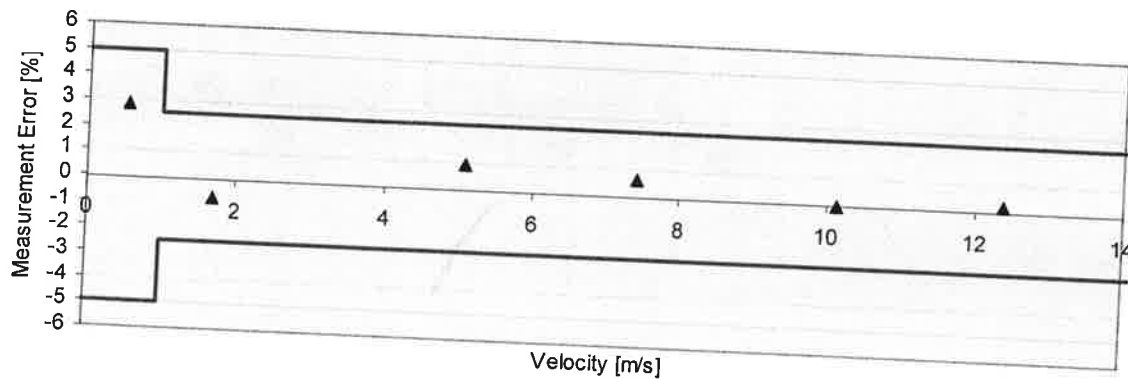

Velocity [m/s]	MUT Velocity [m/s]	Error As Found [%]	Error As Left [%]
0.549	0.566	+2.86	+2.86
1.712	1.699	-0.76	-0.76
5.078	5.126	+0.94	+0.94
7.418	7.468	+0.67	+0.67
10.139	10.130	-0.10	-0.10
12.362	12.381	+0.16	+0.16
		Average Error [%]	+0.627

METER FACTOR: 0.950

TEST DATE: 30-JAN-2015

ISSUED BY: JAY APELES